


Electronic Cigarette Liquid on Rtx®-VMS (Hydrogen)

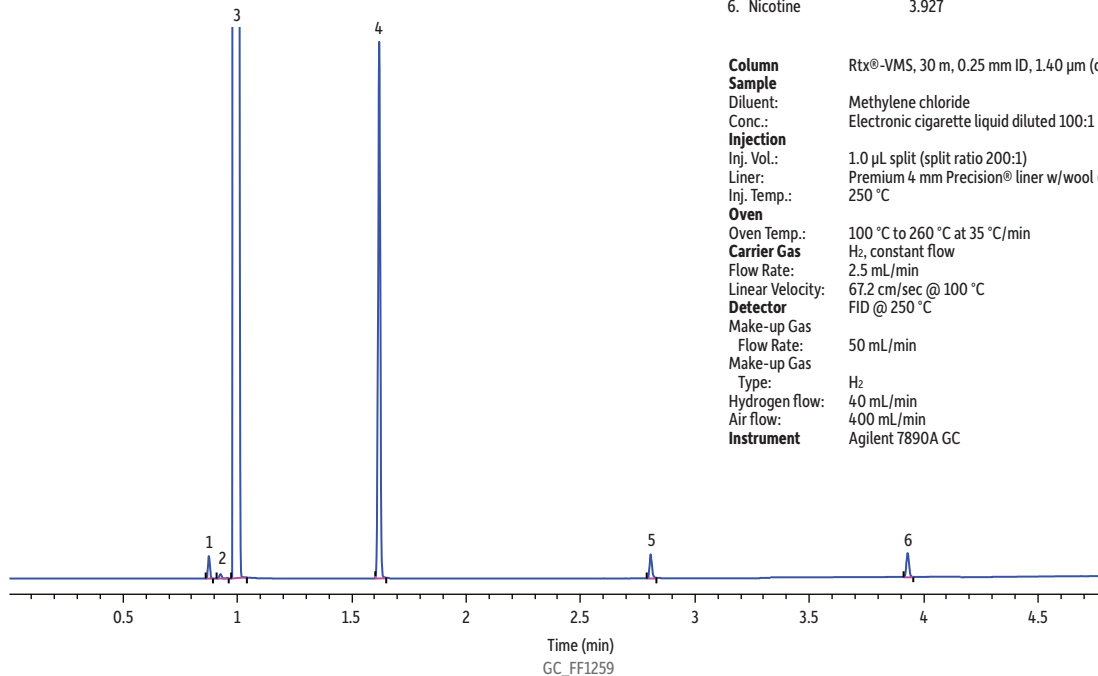

Peaks	ta (min)
1. Methanol	0.875
2. Ethanol	0.926
3. Methylene chloride	0.987
4. Propylene glycol	1.619
5. Glycerin	2.805
6. Nicotine	3.927

Column Rtx®-VMS, 30 m, 0.25 mm ID, 1.40 µm (cat.# 19915)
Sample
Diluent: Methylene chloride
Conc.: Electronic cigarette liquid diluted 100:1
Injection
Inj. Vol.: 1.0 µL split (split ratio 200:1)
Liner: Premium 4 mm Precision® liner w/wool (cat.# 23305.5)
Inj. Temp.: 250 °C
Oven
Oven Temp.: 100 °C to 260 °C at 35 °C/min
Carrier Gas H₂, constant flow
Flow Rate: 2.5 mL/min
Linear Velocity: 67.2 cm/sec @ 100 °C
Detector FID @ 250 °C
Make-up Gas
Flow Rate: 50 mL/min
Make-up Gas
Type: H₂
Hydrogen flow: 40 mL/min
Air flow: 4.00 mL/min
Instrument Agilent 7890A GC