


(±)-1-Octen-3-ol on Rt-βDEXsa

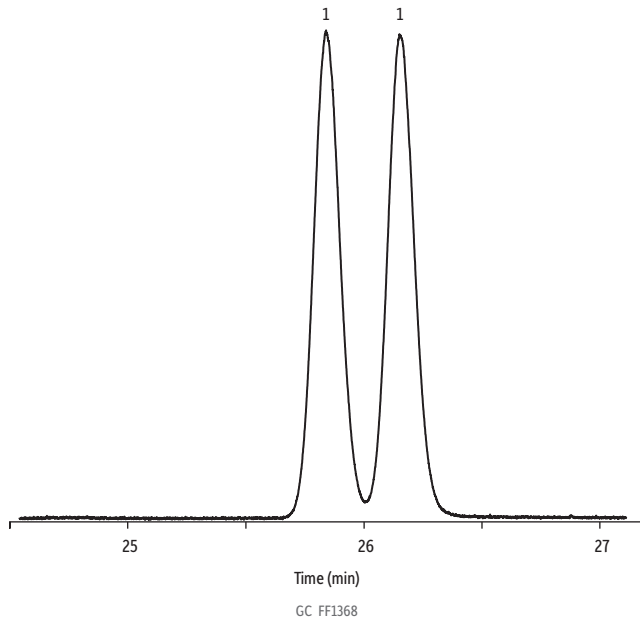

Peaks	tn 1	tn 2
1. (±)-1-Octen-3-ol	25.840	26.153

Column	Rt-βDEXsa, 30 m, 0.32 mm ID, 0.25 μm (cat.# 13108)
Standard/Sample	(±)-1-Octen-3-ol
Diluent:	Acetone
Conc.:	890 μg/mL
Injection	
Inj. Vol.:	1 μL split (split ratio 100:1)
Liner:	Topaz 4.0 mm ID Precision inlet liner w/ wool (cat.# 23305)
Inj. Temp.:	210 °C
Oven	
Oven Temp.:	40 °C (hold 1 min) to 230 °C at 2 °C/min (hold 3 min)
Carrier Gas	H ₂ , constant flow
Linear Velocity:	80 cm/sec @ 40 °C
Detector	FID @ 230 °C
Constant Column +	
Constant Make-up:	51.4 mL/min
Make-up Gas Type:	N ₂
Hydrogen flow:	40 mL/min
Air flow:	400 mL/min
Data Rate:	50 Hz
Instrument	Agilent 7890A GC
Sample Preparation	(±)-1-Octen-3-ol (neat) was dissolved in acetone to a final concentration of 890 ppm in 2 mL, screw-thread vials (cat.# 21143), and capped with short-cap, screw-vial closures (cat.# 24495).
Notes	Enantiomeric resolution of (±)-1-octen-3-ol was 2.0.