


## Now Foods Figure 6: Compared Traditional 5sil Columns to RMX-5Sil MS for Fipronil in Rice at 10 ppb

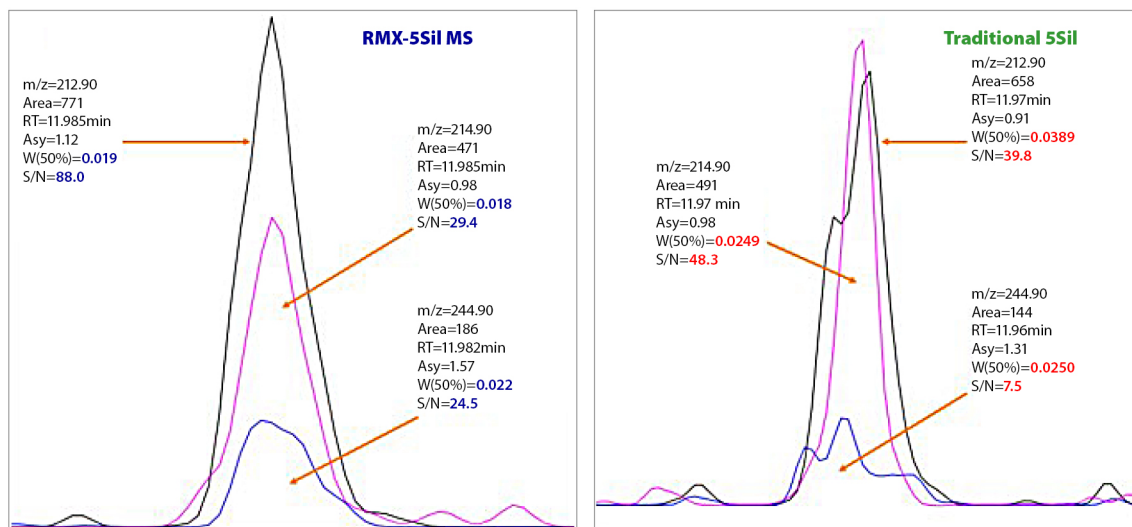

GC\_F50623

Peaks	tr (min)	Conc. (ng/mL)	Precursor	Product	Collision Energy
1. Fipronil	11.88	10	366.9	212.9	28
2. Fipronil	11.88	10	366.9	244.9	20
3. Fipronil	11.88	10	368.8	214.9	30

<b>Column</b>	RMX-5Sil MS GC capillary column with 5 m Integra-Guard & Integra-Transfer Line, 30 m, 0.25 mm ID, 0.25 µm (cat.# 17323-124177)
<b>Standard/Sample</b>	Custom standards
<b>Conc.:</b>	10 pg on-column concentration
<b>Injection</b>	
<b>Inj. Vol.:</b>	1 µL splitless (hold 0.8 min)
<b>Liner:</b>	Topaz 4.0 mm ID single taper liner w/wool (cat.# 23447)
<b>Inj. Temp.:</b>	260 °C
<b>Purge Flow:</b>	60 mL/min
<b>Oven</b>	
<b>Oven Temp.:</b>	40 °C (hold 1.5 min) to 90 °C at 40 °C/min (hold 1.5 min) to 180 °C at 40 °C/min to 250 °C at 10 °C/min to 280 °C at 5 °C/min to 320 °C at 10 °C/min (hold 5 min)
<b>Carrier Gas</b>	He, constant flow
<b>Flow Rate:</b>	1.4 mL/min
<b>Linear Velocity:</b>	32 cm/sec @ 40 °C
<b>Dead Time:</b>	1.56 min @ 40 °C
<b>Detector</b>	Thermo Scientific TSQ 9610 Triple Quadrupole GC-MS
<b>Transfer Line Temp.:</b>	280 °C
<b>Analyzer Type:</b>	Quadrupole
<b>Tune Type:</b>	PFTBA
<b>Ionization Mode:</b>	EI
<b>Instrument</b>	Thermo Scientific Trace 1610 GC
<b>Acknowledgement</b>	NOW Foods