


Impact of MS Scan Rate on Peak Shape and Area

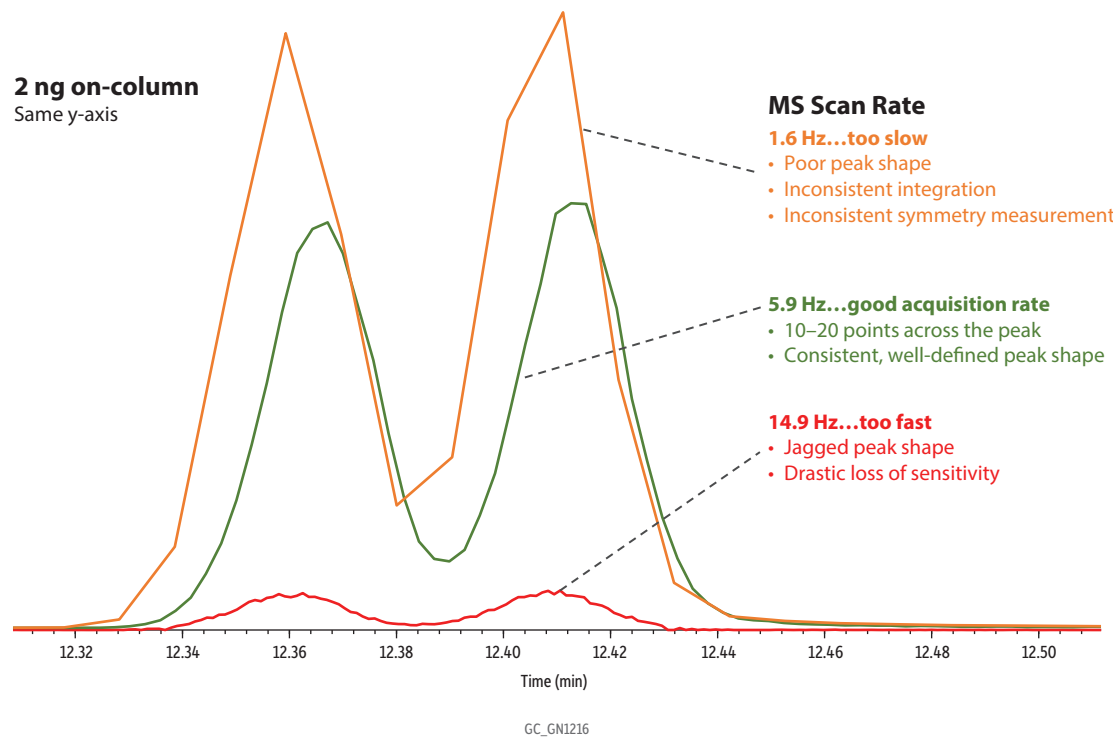

Peaks
1. Benzo[b]fluoranthene
2. Benzo[k]fluoranthene

Column
Injection
Oven
Detector
Mode:
Instrument

split
MS
Scan
Agilent 7890B GC & 5977A MSD