Total Glycerin in Biodiesel
MXT®-Biodiesel TG

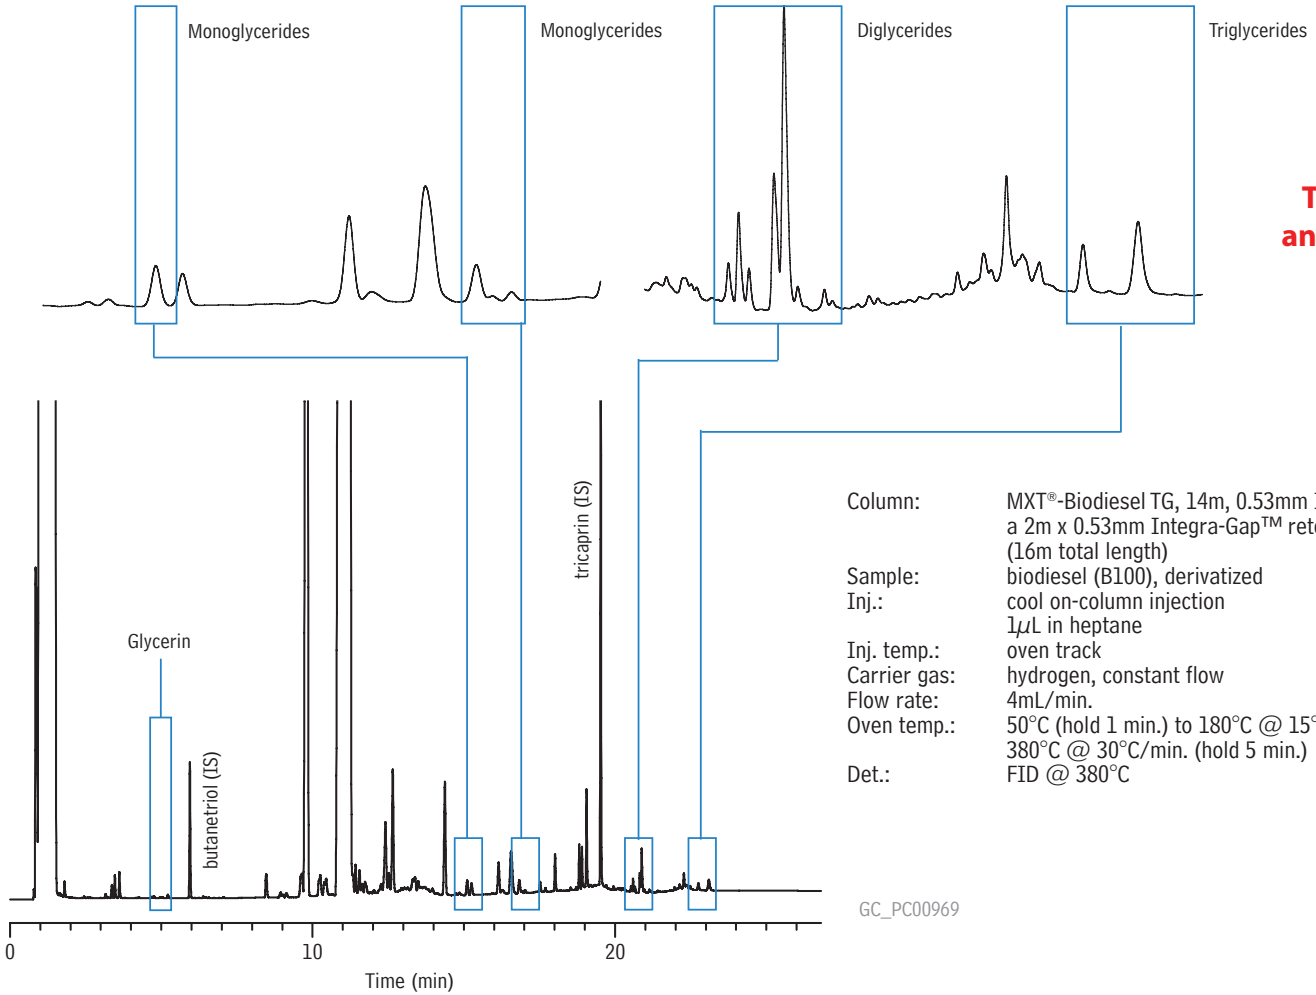

The best solution for analyzing total glycerin in biodiesel!

Column:	MXT®-Biodiesel TG, 14m, 0.53mm ID, 0.16µm (cat.# 70289) with a 2m x 0.53mm Integra-Gap™ retention gap (16m total length)
Sample:	biodiesel (B100), derivatized
Inj.:	cool on-column injection 1µL in heptane
Inj. temp.:	oven track
Carrier gas:	hydrogen, constant flow
Flow rate:	4mL/min.
Oven temp.:	50°C (hold 1 min.) to 180°C @ 15°C/min. to 230°C @ 7°C/min. to 380°C @ 30°C/min. (hold 5 min.)
Det.:	FID @ 380°C

GC_PC00969

Restek Corporation 110 Benner Circle Bellefonte, PA 16823
814-353-1300 • 800-356-1688 • Fax: 814-353-1309 • www.restek.com