


# Psilocin and Psilocybin in Urine on Raptor Biphenyl by Restek's 'Big Pain' Method (CFAR2309-UNV)

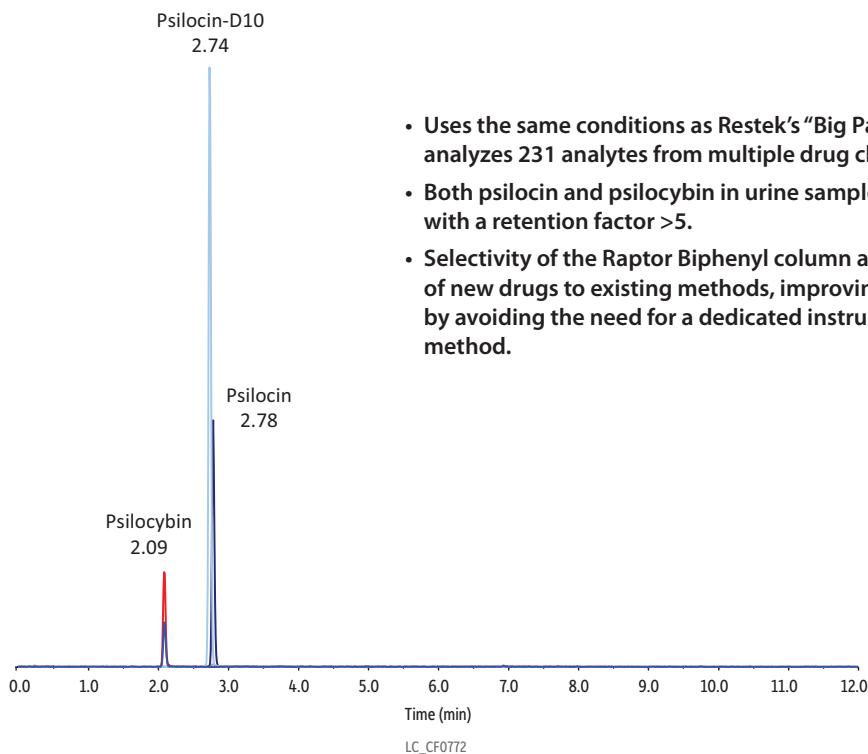

- Uses the same conditions as Restek's "Big Pain" method that analyzes 231 analytes from multiple drug classes.
- Both psilocin and psilocybin in urine samples are separated with a retention factor >5.
- Selectivity of the Raptor Biphenyl column allow the addition of new drugs to existing methods, improving lab productivity by avoiding the need for a dedicated instrument and separate method.

| Peaks           | tr (min) | Conc. (ng/mL) | Precursor Ion | Product Ion 1 | Product Ion 2 |
|-----------------|----------|---------------|---------------|---------------|---------------|
| 1. Psilocybin   | 2.09     | 500           | 285.1         | 205.1         | 240.0         |
| 2. Psilocin-D10 | 2.74     | 200           | 215.1         | 66.1          | -             |
| 3. Psilocin     | 2.78     | 500           | 205.1         | 160.1         | 115.0         |

**Column** Raptor Biphenyl (cat.# 9309A12)  
 Dimensions: 100 mm x 2.1 mm ID  
 Particle Size: 2.7 µm  
 Pore Size: 90 Å  
 Guard Column: Raptor Biphenyl EXP guard column cartridge 5.0 mm, 2.1 mm ID, 2.7 µm (cat.# 9309A0252)  
 Temp.: 30 °C

**Standard/Sample**  
 Diluent: Water, 0.1% formic acid + 2 mM ammonium formate  
 Conc.: 500 ng/mL  
 Inj. Vol.: 5 µL

**Mobile Phase**  
 A: Water, 0.1% formic acid + 2 mM ammonium formate  
 B: Methanol, 0.1% formic acid + 2 mM ammonium formate

| Time (min) | Flow (mL/min) | %A | %B  |
|------------|---------------|----|-----|
| 0.00       | 0.6           | 95 | 5   |
| 9.00       | 0.6           | 0  | 100 |
| 10.00      | 0.6           | 0  | 100 |
| 10.01      | 0.6           | 95 | 5   |
| 12.00      | 0.6           | 95 | 5   |

**Detector** MS/MS  
 Ion Source: Electrospray  
 Ion Mode: ESI+  
 Mode: MRM  
**Instrument** HPLC

**Sample Preparation**  
 A 500 ng/mL standard mix of psilocin and psilocybin was prepared in pooled urine. A 50 µL aliquot was taken from the standard and mixed with 10 µL of internal standard (psilocin-D10, 20 µg/mL) and 100 µL of methanol. The mixture was vortexed at 3000 rpm for 10 seconds and centrifuged at 4300 rpm for 10 minutes at 10 °C. After centrifugation, 100 µL of the supernatant was diluted with 900 µL (20-fold dilution) of water containing 0.1% formic acid and 2 mM ammonium formate (mobile phase A) and injected for LC-MS/MS analysis.